




CERTIFIED CALIBRATION CHART

For Customer Use Only:		DATE CALIBRATION CYCLE BEGINS _____		CALIBRATION DUE DATE _____	
NAGANO KEIKI CO LTD CUSTOMER NAME			N001141533 CUSTOMER ORDER No		13 ITEM No
NAGANO KEIKI CO LTD SHIP TO / END USER NAME				N001141530 END USER PO	
10387972 ORDER No.	13 LINE No.	DG253HL0NAMR4L.5MP&V-#5094C4 DESCRIPTION			15101409022 SERIAL No
-0.1 MIN. RANGE	0.5 MAX. RANGE	psi UNITS	0.25% ACCURACY		

TRUE VALUE	INCREASE		DECREASE	
	VALUE	% ERROR	VALUE	% ERROR
-0.10	-0.1001	-0.02%	-0.1000	0.00%
-0.05	-0.0500	0.00%	-0.0500	0.00%
0.00	0.0000	0.00%	0.0001	0.02%
0.25	0.2498	-0.03%	0.2500	0.00%
0.50	0.5000	0.00%	0.5000	0.00%

EQUIPMENT USED FOR INSPECTION	
Pressure Standard Used :	Digigauge
Serial /ID Number :	1073
Range :	100psi
Accuracy :	0.05%
Date Calibrated :	09/10/2015
Due Date of Calibration:	03/10/2016
<small>Tested in accordance with ASME B 40.100:2013 Accuracy of Unit is traceable to N.I.S.T</small>	

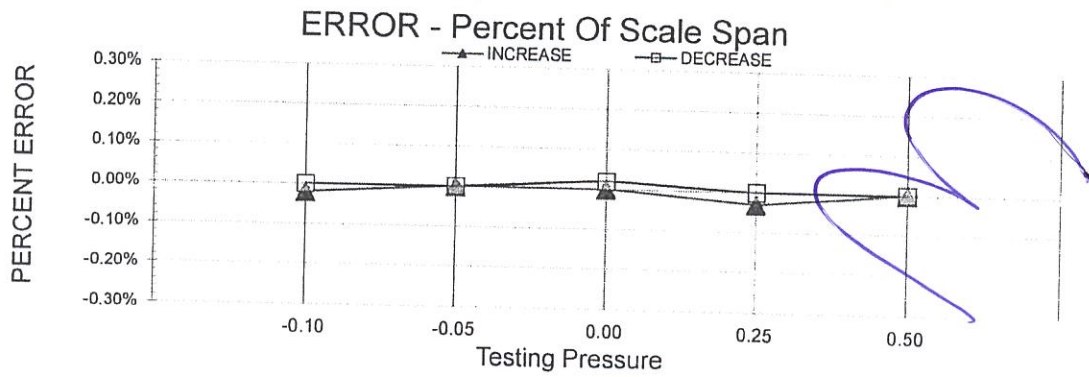

All standards used in this calibration are maintained in accordance with the latest revisions of ANSI/NCSL Z540-1 and ISO-10012

October 16, 2015	9607	Certified By:
DATE OF CALIBRATION at ASHCROFT® INC.	TESTED BY	

This certificate shall not be reproduced, except fully, with a written permission from ASHCROFT® INC.

250 East Main Street - Stratford, CT 06614-5145 - Phone: 203-378-8281 - www.ashcroft.com